

Instructions for use

MASTERmatic LUX M07 L - 1.009.3610

MASTERmatic LUX M20 L - 1.009.3620

MASTERmatic LUX M29 L - 1.009.3580



KaVo. Dental Excellence.

Distributed by:

KaVo Dental GmbH
Bismarckring 39
D-88400 Biberach
Phone +49 7351 56-0
Fax +49 7351 56-1488

Manufacturer:

Kaltenbach & Voigt GmbH
Bismarckring 39
D-88400 Biberach
www.kavo.com



Table of contents

1	User instructions.....	6
2	Safety.....	8
2.1	Description of safety instructions.....	8
2.2	Safety instructions.....	11
3	Product description.....	16
3.1	Purpose – Intended use.....	19
3.2	Technical Specifications M07 L.....	21
3.3	Technical Specifications M20 L.....	22
3.4	Technical Specifications M29 L.....	23
3.5	Transportation and storage conditions.....	24
4	Start up and shut down.....	26
4.1	Check the amount of water.....	27
5	Operation.....	30
5.1	Attach the medical device.....	30
5.2	Remove the medical device.....	32

5.3	Insert the INTRA LUX	33
5.4	Remove the INTRA LUX	34
6	Troubleshooting.....	35
6.1	Check for malfunctions.....	35
6.2	Troubleshooting.....	38
6.2.1	Replacing the O-rings.....	38
6.2.2	Cleaning the spray nozzle.....	39
6.2.3	Changing the water filter.....	41
7	Reprocessing steps in accordance with ISO 17664.....	43
7.1	Preparations at the site of use.....	43
7.2	Cleaning.....	44
7.2.1	Manual cleaning - external.....	45
7.2.2	Automated external cleaning.....	45
7.2.3	Manual cleaning - internal.....	46
7.2.4	Automated internal cleaning.....	48
7.3	Disinfection.....	49

7.3.1	Manual disinfection - external.....	52
7.3.2	Manual disinfection - internal.....	53
7.3.3	Machine disinfection - external and internal.....	54
7.4	Drying.....	55
7.5	Care products and systems - Servicing.....	56
7.5.1	Care with KaVo Spray.....	57
7.5.2	Care with the KaVo SPRAY rotor.....	58
7.5.3	Servicing with KaVo QUATTROcare 2104 / 2104A.....	59
7.5.4	Servicing with KaVo QUATTROcare PLUS 2124 A.....	62
7.5.5	Servicing with KaVo QUATTROcare 2140 A.....	63
7.6	Packaging.....	64
7.7	Sterilisation.....	65
7.8	Storage.....	67
8	Tools and consumables.....	68
9	Warranty terms and conditions.....	70



1 User instructions





Dear User

Congratulations on purchasing this KaVo quality product. By following the instructions below you will be able to work smoothly, economically and safely.

© Copyright by KaVo Dental GmbH

Symbols

	Refer to the chapter on Safety/Warning symbol
	Important information for users and service technicians

	Can be steam-sterilised at 134 °C -1 °C / +4 °C (273 °F -1.6 °F / +7.4 °F)
	Thermodisinfectable
	CE-Zeichen (Communauté Européenne). Ein Produkt mit diesem Zeichen entspricht den Anforderungen der anwendbaren EG-Richtlinie.
	Action request

Target group

This document is intended for dentists and their assistants. The section on starting up is also intended for service technicians.

2 Safety

2.1 Description of safety instructions



Warning symbol

Structure



DANGER

The introduction describes the type and source of the hazard.

This section describes potential consequences of non-compliance.

The optional step includes necessary measures for hazard prevention.



Description of hazard levels

The safety instructions listed here, together with the three levels of danger will help avert property damage and injury.



 **CAUTION**

CAUTION

indicates a hazardous situation that can cause damage to property or mild to moderate injuries.

**⚠ WARNING****WARNING**

indicates a hazardous situation that can lead to serious or fatal injury.

**⚠ DANGER****DANGER**

indicates a maximal hazard due to a situation that can directly cause death or fatal injury.

2.2 Safety instructions



WARNING

Hazard from incorrectly reconditioned products.

An infection hazard exists from contaminated products.

Take suitable personal protective measures.



WARNING

Hazards for the care provider and the patient

In the case of damage, irregular running noise, excessive vibration, untypical warming or when the cutter or grinder cannot be held.

Do not use further and notify Service.



CAUTION

Hazard from use as a light probe.

Do not use the device as a light probe since the rotating cutters or grinders can cause injury.

Use an appropriate light probe for additional illumination of the oral cavity or site of preparation.



CAUTION

Premature wear and malfunctioning from improper storage during long periods of nonuse.

Reduced product life.

The medical device should be cleaned, serviced and stored in a dry location, according to instructions, before long periods of nonuse.

The following individuals are authorized to repair and service KaVo products:


Technicians at KaVo branches throughout the world

Technicians specially trained by KaVo


To ensure proper function, the medical device must be set up according to the reprocessing methods described in the KaVo Instructions for Use, and the care products and care systems described therein must be used. KaVo recommends specifying a service interval at the dental office for a licensed shop to clean, service and check the functioning of the medical device. This service interval depends on the frequency of use and should be adjusted accordingly.

Service may only be carried out by KaVo-trained repair shops using original KaVo replacement parts.


3 Product description

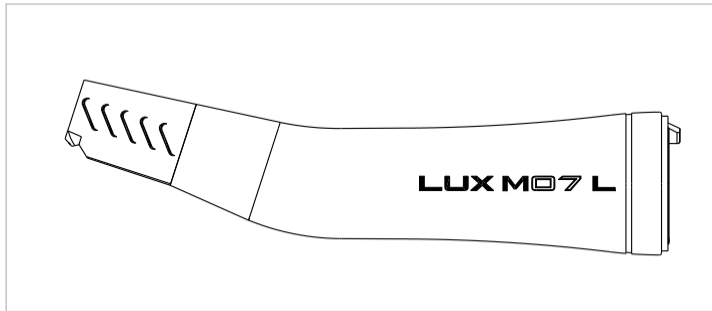

MASTERmatic LUX M07 L (Mat no. 1.009.3610)

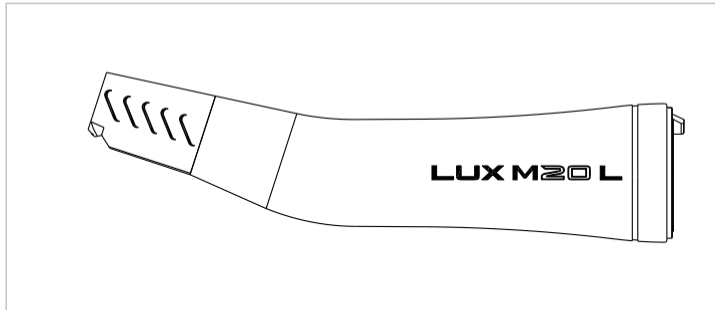

MASTE Rmatic LUX M20 L (Mat no. 1.009.3620)

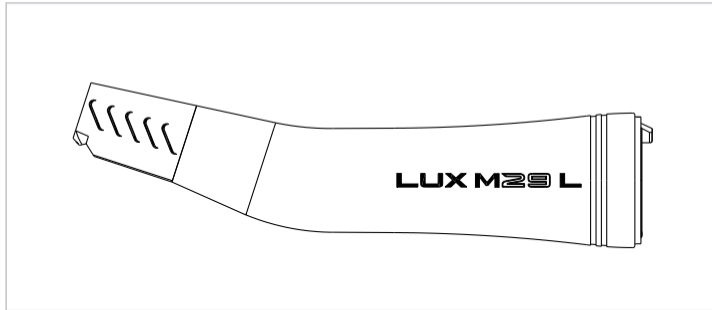

MASTERmatic LUX M29 L (Mat no. 1.009.3580)

3.1 Purpose – Intended use

Indications for use:

This medical device is

intended for dental treatment only. All other types of use or modifications of the product are not permitted and can be hazardous. The medical device, used in combination with the respective handpiece heads, is intended for the following applications: Removal of carious material, cavity and crown preparations, removal of fillings, processing of tooth and restoration surfaces.

A medical device according to relevant national statutory regulations.

Proper use:

According to these regulations, this medical device may only be used for the described application by a knowledgeable user. You need to comply with the following:

- the applicable health and safety regulations
- the applicable accident prevention regulations
- these Instructions for use

According to these regulations, the user is required to:

- only use equipment that is operating correctly,
- adhere to the specified intended use
- protect him or herself, the patient and third parties from danger, and

avoid contamination from the product

3.2 Technical Specifications M07 L

Drive speed	max. 40,000 rpm
Step-down ratio	2.7 : 1
Maximum speed:	max. 15,000 rpm
identification	1 green ring
Spray water pressure	0.8 to 2.0 bar (12 to 29 psi)
Spray air pressure	1.0 to 2.0 bar (15 to 29 psi)
Spray air quantity	min. 1.5 NI/min (at 2 bar)
Cooling air flow	5.5 to 9.5 NI/min

All INTRA heads and INTRA LUX heads can be used.

The shank can be mounted on all INTRAmatic motors and motors fitted with a connection in accordance with ISO 3964 / DIN 13940.

3.3 Technical Specifications M20 L

Drive speed	max. 40,000 rpm
Step-down ratio	1 : 1
Maximum speed:	max. 40,000 rpm
Identification	1 blue ring
Spray water pressure	0.8 to 2.0 bar (12 to 29 psi)
Spray air pressure	1.0 to 2.0 bar (15 to 29 psi)
Spray air quantity	min. 1.5 NI/min (at 2 bar)
Cooling air flow	5.5 to 9.5 NI/min

All INTRA heads and INTRA LUX heads can be used.

The shank can be mounted on all INTRAmatic motors and motors fitted with a connection in accordance with ISO 3964 /DIN 13940.

3.4 Technical Specifications M29 L

Drive speed	max. 40,000 rpm
Step-down ratio	7.4 : 1
Maximum speed:	max. 5,000 min ⁻¹
identification	2 green rings
Spray water pressure	0.8 to 2.0 bar (12 to 29 psi)
Spray air pressure	1.0 to 2.0 bar (15 to 29 psi)
Spray air quantity	min. 1.5 NI/min (at 2 bar)
Cooling air flow	5.5 to 9.5 NI/min

All INTRA heads and INTRA LUX heads can be used.

The shank can be mounted on all INTRAmatic motors and motors fitted with a connection in accordance with ISO 3964 / DIN 13940.

3.5 Transportation and storage conditions

CAUTION






It is hazardous to start up the medical device after it has been stored strongly refrigerated.

This can cause the medical device to malfunction.

Prior to start-up, very cold products must be heated to a temperature of 20°C to 25°C (68°F to 77°F).



Temperature: -20°C to +70°C (-4°F to +158°F)

	Relative humidity: 5% RH to 95% RH absence of condensation
	Air pressure: 700 hPa to 1060 hPa (10 psi to 15 psi)
	Protect from moisture

4 Start up and shut down



WARNING

Hazard from non-sterile products.

Infection hazard for care provider and patient

Before first use and after each use, prepare and sterilise the medical device and accessories accordingly.



WARNING

Disposal of the product in the appropriate manner.

Prior to disposal, the product and accessories must be appropriately prepared or sterilised if this is necessary.

4.1 Check the amount of water



CAUTION

Overheating of the tooth due to insufficient amount of cooling water.

Thermal damage to the dental pulp.

Adjust the water amount for the spray cooling to a minimum of 50 ml/min!




CAUTION

Hazard from insufficient spray water.

Insufficient spray water can cause the medical device to overheat and damage the tooth.

Check the spray water channels and clean the spray nozzles with the nozzle needle **Mat no. 0.410.0921** if necessary.

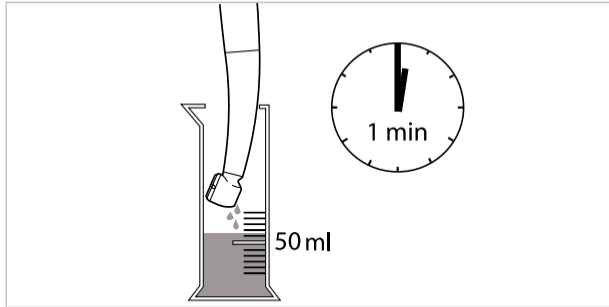

5 Operation

5.1 Attach the medical device



WARNING

Release of the medical device during treatment

A medical device that is not properly locked in place can release from the motor coupling and fall off.

Carefully pull on it before each treatment to ensure that the medical device is securely locked on the motor coupling.



CAUTION

Removing and attaching the handpiece while the drive motor is rotating.

Damage to the catch.

Never attach or remove the reducing shank while the device is rotating!

Attach medical device to the (LUX) motor coupling and turn it until the latch audibly snaps into place.

Pull on the medical device to make sure that it is securely affixed to the coupling.

5.2 Remove the medical device

Unlock the medical device from the motor coupling and then pull it off along its axis.

5.3 Insert the INTRA LUX

CAUTION

Loosening of the medical device during treatment

If the head is not properly locked in place, it can fall out during treatment.

Do not mount or remove the head while rotating. Before each treatment, check that the head is firmly seated and that the clamping ring is tight.



Rotate the clamping ring in the direction of the arrow to the stop.

Insert the head to the stop. Make sure that the catches are properly seated.

Rotate the clamping ring in the opposite direction (-> close) and tighten it

5.4 Remove the INTRA LUX

Rotate the clamping ring in the direction of the arrow to the stop.

6 Troubleshooting

6.1 Check for malfunctions



CAUTION

Missing or damaged O-rings.

Malfunctions and premature failure.

Make sure that all O-rings are on the coupling and undamaged.



CAUTION

Heating of the product

Burns or product damage from overheating.

Do not use the product if it is irregularly heated.

The medical device is too hot while idling:

Check the amount of cooling air.

The medical device is too hot while working:

Caring for the medical device.

When the speed drops or is uneven:

Caring for the medical device.

An O-ring is missing on the motor coupling:

Replace O-ring.

6.2 Troubleshooting

6.2.1 Replacing the O-rings



CAUTION

Hazard from improper care of the O-rings.

Malfunctions or complete failure of the medical device.

Do not use Vaseline or other grease or oil.



Note

The O-ring on the coupling may only be lubricated with a cotton ball wet with KAVO spray.

Press the O-ring between your fingers to form a loop.

Shove the O-ring to the front, and remove it.

Insert new O-rings into the grooves.

6.2.2 Cleaning the spray nozzle



CAUTION

Hazard from insufficient spray water.

Overheating of the medical device and damage to the tooth.

Check the spray water channels and clean the spray nozzles with the nozzle needle **Mat no. 0.410.0921** if necessary.

Check the water filter and exchange if necessary.



Use the nozzle needle (**Mat no. 0.410.0921**) to free the water passage in the spray nozzles.

6.2.3 Changing the water filter




CAUTION

Hazard from insufficient spray water.

Insufficient spray water can cause the medical device to overheat and damage the tooth.

Check the filter and exchange if necessary.

Check the spray water channels and clean the spray nozzles with the nozzle needle **Mat no. 0.410.0921** if necessary.



Remove all residual cement, composite or blood without delay.

Reprocess the medical device as soon as possible after treatment

The medical device must be dry when transported for reconditioning.

Do not place it in a solution or similar.

7.2 Cleaning



CAUTION

Malfunctions from cleaning in the ultrasonic unit

Defects in the product


Only clean manually or in a thermodisinfectant.

7.2.1 Manual cleaning - external

Accessories required:

Tap water $30\text{ }^{\circ}\text{C} \pm 5\text{ }^{\circ}\text{C}$ ($86\text{ }^{\circ}\text{F} \pm 10\text{ }^{\circ}\text{F}$)

Brush, e.g. medium-hard toothbrush



Brush off under flowing tap water.

7.2.2 Automated external cleaning



KaVo recommends washer disinfectors in compliance with EN ISO 15883-1, which are operated using alkaline cleaning agents.

For program settings as well as cleansers and disinfectants to be used, please refer to the Instructions for Use of the thermodisinfectors.

In order to prevent negative effects on the medical device, make sure that the interior and the exterior of the medical device are dry after completion of the cycle, and then grease it immediately with servicing agents from the KaVo care system.

7.2.3 Manual cleaning - internal

Validated interior cleaning (residual protein removal) can only be accomplished with KaVo CLEANspray and KaVo DRYspray.

Cover the medical device with the KaVo CLEANpac bag, and place it on the corresponding care adapter. Press the spray button three times for 2 seconds each time. Remove the medical device from the spray attachment and let the cleaner work for one minute.

Afterwards, rinse for 3-5 seconds with KaVo DRY spray.

See also:

 KaVo CLEANspray /KaVo DRYspray Instructions for Use



Note

KaVo CLEANspray and KaVo DRY spray for manual interior cleaning are only available in the following countries:

Germany, Austria, Switzerland, Italy, Spain, Portugal, France, Luxembourg, Belgium, Netherlands, United Kingdom, Denmark, Sweden, Finland and Norway.

In other countries interior cleaning can only be carried out with thermodisinfectors in accordance with EN ISO 15883-1.

7.2.4 Automated internal cleaning



KaVo recommends washer disinfectors in compliance with EN ISO 15883-1, which are operated using alkaline cleaning agents.

For programme settings as well as cleansers and disinfectants to be used, please refer to the Instructions for Use of the washer disinfectator.

In order to prevent negative effects on the medical device, make sure that the interior and the exterior of the medical device are dry after completion of the cycle, and then grease it immediately with servicing agents from the KaVo care system.

7.3 Disinfection



WARNING

Hazard due to incomplete disinfection.

Principally, KaVo recommends carrying out a final disinfection of the un packaged item if complete disinfection cannot be guaranteed without this measure.



CAUTION

Malfunctioning from using a disinfectant bath or disinfectant containing chlorine.

Defects in the product

Only disinfect in a thermodisinfectior or manually.



⚠ CAUTION

Malfunctioning from using the disinfectant bath or chlorine-containing disinfectants.

Defects in the device.

Do not use an ultrasonic bath.



⚠ CAUTION

Never use alkaline or chlorine-containing disinfectants.

The saline solution corrodes the metal parts.

Immediately remove all residue.

7.3.1 Manual disinfection - external



KaVo recommends the following products based on material compatibility. The microbiological efficacy must be ensured by the disinfectant manufacturer.

Mikrozid AF made by Schülke & Mayr (liquid or cloths)

FD 322 made by Dürr

CaviCide made by Metrex

Consumables required:

Cloths for wiping off the medical device.

Spray the disinfectant on a cloth, then wipe down the medical device and allow the disinfectant to act according to the instructions of the disinfectant manufacturer.

Follow the instructions for use of the disinfectant

7.3.2 Manual disinfection - internal

The efficacy of manual internal disinfection must be demonstrated by the manufacturer of the disinfection agent. With KaVo products, use only disinfection agents that have been released by KaVo with respect to the compatibility of materials (e.g. WL-cid /made by ALPRO).

Blow off with compressed air until no water drops are visible.

Immediately after internal disinfection, lubricate the KaVo medical device immediately with care agents from the KaVo care system.

7.3.3 Machine disinfection - external and internal



KaVo recommends washer disinfectors in compliance with EN ISO 15883-1, which are operated using alkaline cleaning agents.

For programme settings as well as cleansers and disinfectants to be used, please refer to the Instructions for Use of the washer disinfector.

In order to prevent negative effects on the medical device, make sure that the interior and the exterior of the medical device are dry after completion of the cycle, and then grease it immediately with servicing agents from the KaVo care system.

7.4 Drying

Manual Drying

Blow off the outside and inside with compressed air until water drops are no longer visible.

Automatic Drying

The drying procedure is usually a part of the cleaning program of the thermodisinfectors.

Follow the instructions for use of the thermodisinfectors.

7.5 Care products and systems - Servicing



CAUTION

Premature wear and malfunctions from improper servicing and care.

Reduced product life.

Perform proper care regularly!



Note

KaVo only guarantees that its products will function properly when the care products are used that are listed as accessories since they were tested for proper use on our products.


7.5.1 Care with KaVo Spray



Note

The shank can be serviced either alone or with a head attached to it


KaVo recommends servicing the product as part of the reprocessing after each use, i.e. after each cleaning, disinfection, and before each sterilisation.



Cover the product with the Cleanpac bag.

Plug the product onto the cannula, and press the spray button for one second.

7.5.2 Care with the KaVo SPRAY rotor



Note

The shank can be serviced either alone or with a head attached to it

Place the product on the appropriate coupling of the KaVo SPRAY rotor and cover it with a Cleanpac bag.

Servicing the product

See also:

 Instructions for use KaVo SPRAYrotor

7.5.3 Servicing with KaVo QUATTROcare 2104 / 2104A



Note

The shank can be serviced either alone or with a head attached to it

Cleaning and servicing unit with expansion pressure for effective cleaning and care.



Note

QUATTROcare 2104 / 2104 A is no longer included in the current delivery programme.


Follow-up products:

QUATTROcare PLUS 2124 A

QUATTROcare CLEAN 2140 A

Servicing and cleaning device with expansion pressure for the interior cleaning of inorganic residues and optimum care.

(no validated cleaning of the interior in accordance with German RKI requirements)



KaVo recommends servicing the product as part of the reprocessing after each use, i.e. after each cleaning, disinfection, and before each sterilisation.

Remove the cutter or grinder.

Servicing the product.

See also:

 Instructions for use KaVo QUATTROcare 2104 / 2104A

7.5.4 Servicing with KaVo QUATTROcare PLUS 2124 A



Note

The shank can be serviced either alone or with a head attached to it

Servicing and cleaning device with expansion pressure for the interior cleaning of inorganic residues and optimum care.

(no validated cleaning of the interior in accordance with German RKI requirements)



Remove the cutter or grinder.


Servicing the product in the QUATTROcare PLUS.

See also:

 Instructions for Use KaVo QUATTROcare PLUS 2124 A

7.5.5 Servicing with KaVo QUATTROcare 2140 A

Programme-controlled cleaning and servicing device for perfect servicing of handpieces and turbines.



Remove the cutter or grinder.

Servicing the product in QUATTROcare CLEAN.

See also:

 Instructions for use KaVo QUATTROcare CLEAN 2140 A

7.6 Packaging**Note**

The sterilisation bag must be large enough for the handpiece so that the bag is not stretched.

The quality and use of the sterilisation packaging must satisfy applicable standards and be suitable for the sterilisation procedure!

Weld each medical device individually in a sterilised item package!

7.7 Sterilisation

Sterilisation in a steam steriliser (autoclave) in accordance with EN 13060 / ISO 17665-1



CAUTION

Premature wear and malfunctions from improper servicing and care.

Reduced product life.

Before each sterilisation cycle, service the medical device with KaVo care products.



CAUTION

Contact corrosion due to moisture.

Damage to product

Immediately remove the product from the steam steriliser after the sterilisation cycle!

The KaVo medical device has a maximum temperature resistance of up to 138 (280.4 °F).

Select a suitable procedure (depending on the available autoclave) from the following sterilisation processes:

Autoclave with three times pre-vacuum:

- at least 3 minutes at 134 °C -1 °C / +4 °C (273 °F -1.6 °F / +7.4 °F)

Autoclave using the gravity method:

- at least 10 minutes at 134 °C -1 °C / +4 °C (273 °F -1.6 °F / +7.4 °F)
Use according to the manufacturer's Instructions for Use.

7.8 Storage

Reprocessed products should be stored protected from dust with minimum exposure to germs in a dry, dark and cool space.



Note

Comply with the expiry date of the sterilised items.

8 Tools and consumables

Available from dental suppliers.

Material summary	Mat No.
Instrument stand 2151	0.411.9501
Cleanpac 10 units	0.411.9691
Cellulose pad 100 units	0.411.9862
Nozzle pin	0.410.0921
Replacement filter	1.002.0271
Wrench	1.002.0321
O-ring	0.200.6120

Material summary	Mat no.
KaVo CLEANspray 2110 P	1.007.0579
KaVo DRYspray 2117 P	1.007.0580
KaVo Spray 2112 A	0.411.9640
ROTA spray 2 2142 A	0.411.7520
QUATTROcare plus Spray 2140 P	1.005.4525

9 Warranty terms and conditions

The following warranty conditions apply to this KaVo medical device:

KaVo provides the end customer with a warranty of proper function and guarantees zero defects in respect of material and processing for a period of 24 months from date of invoice, subject to the following conditions:

In case of justified complaints, KaVo will honour its warranty with a free replacement or repair. Other claims of any nature whatsoever, in particular with respect to compensation, are excluded. In the event of default, gross negligence or intent, this shall only apply in the absence of mandatory legal regulations to the contrary.

KaVo cannot be held liable for defects and their consequences that have arisen or may arise from natural wear, improper handling, cleaning or maintenance, non-compliance with operating, maintenance or connection instructions, calcination or corrosion, contaminated air or water supplies or chemical or electrical factors deemed abnormal or impermissible in accord

ance with KaVo's instructions for use or other manufacturer's instructions. The warranty does not usually cover lamps, light conductors made of glass and glass fibres, glassware, rubber parts and the colourfastness of plastic parts.

Defects or their consequences that can be attributed to interventions on or changes made to the product by the customer or a third party not authorised by KaVo are excluded from the warranty.

Service warranty claims will only be accepted if the product is submitted along with proof of purchase in the form of a copy of the invoice/delivery note. The dealer, purchase date, unit number or type and serial number must be clearly visible on this document.

1.010.9104 · kb · 20150211 - 02 · en



KaVo. Dental Excellence.